


COVID Application



Serology test solution

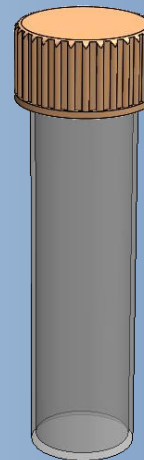

Tube BIOER BSC82X1-A
Ø15,5 x 56 mm

 **RIEGER**
Industrievertretungen GmbH
www.rieger-iv.at




Wir sind für Sie da:
E-Mail: office@rieger-iv.at
Telefon: +43(1) 728 00 52
Fax: +43(1) 728 69 16
Rustenschacher Allee 10
1020 Wien, Austria

ST2004006A

LISA + RX 625 + B625

SPECIAL ADAPTER 2T2-COVID



- 60 tubes / cycle
- Radius 177mm
- Max 5100 rpm / 5147g

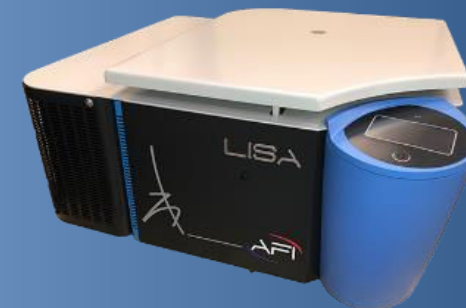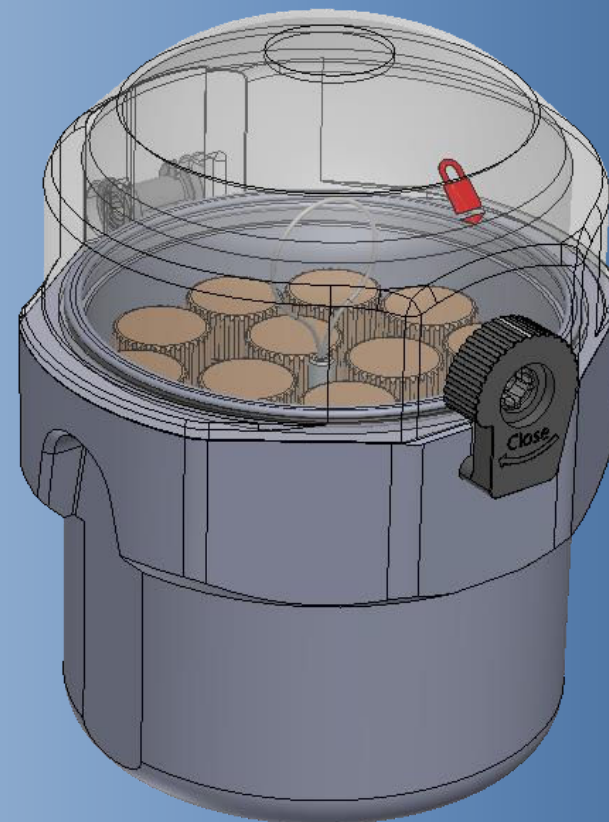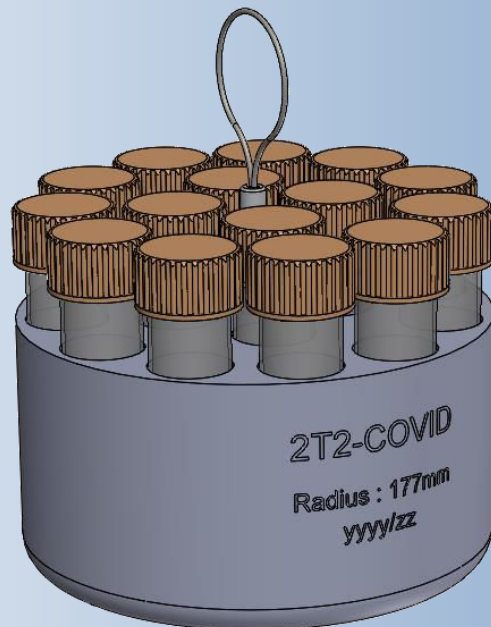

LOREENA + RX 750+ B750

SPECIAL ADAPTER 3T2-COVID

- **76** tubes / cycle
- Radius 193mm
- Max 4650 rpm / 4665g


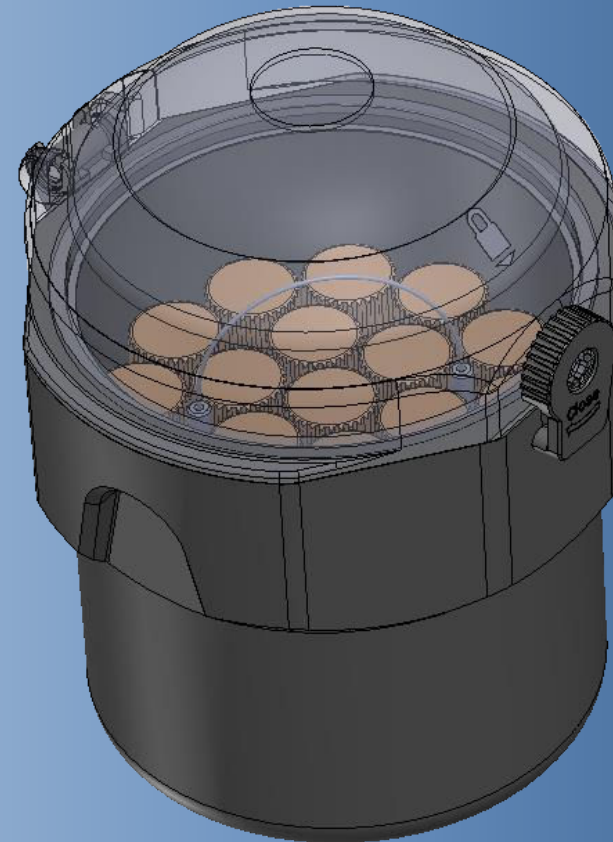
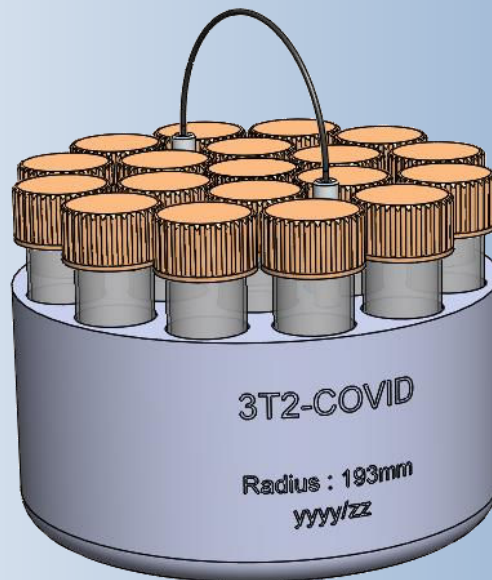


LOREENA + RX1000 + B1000



SPECIAL ADAPTER 4T2-COVID

- 96 tubes / cycle
- Radius 190mm
- Max 3500 rpm / 2602g

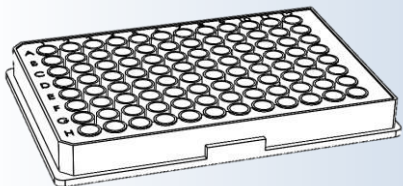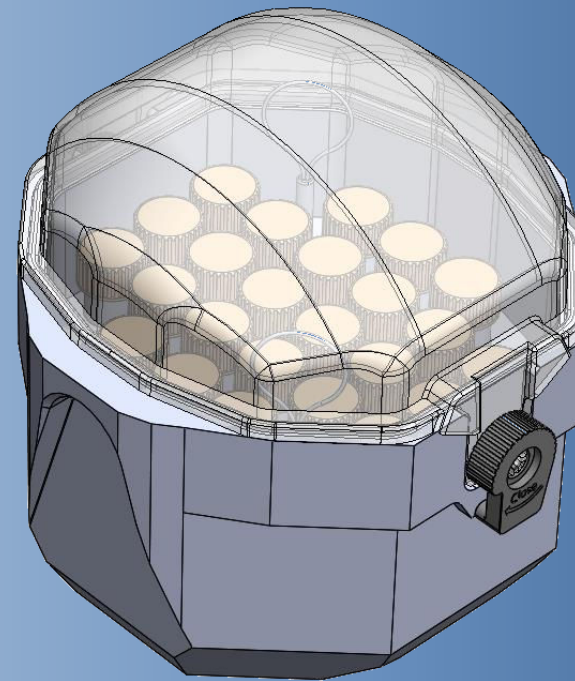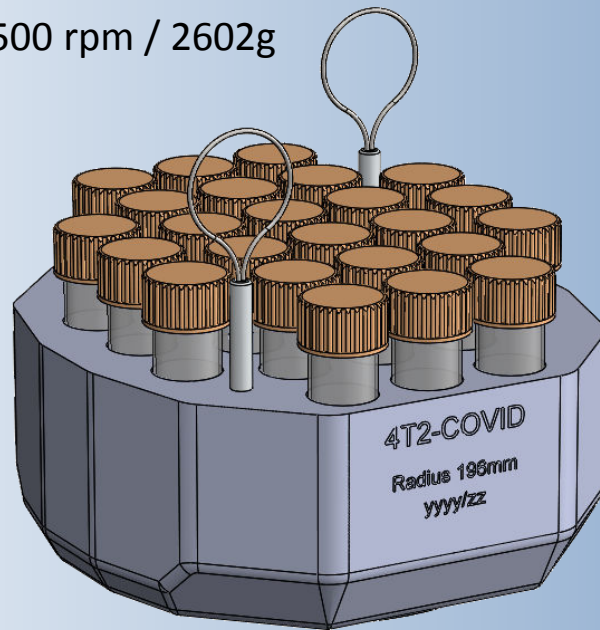

96 tubes to 96 wells
Tracability secured process



+ d'informations

www.afigroups.com

+33 2 43 06 15 19

contact@afigroups.com



ATALIA
Certification

ISO 13485 : 2016
N° ATA 028/2017



ATALIA
Certification

ISO 9001 : 2015
N° ATA 032/2017

